


First order Raman spectrum of a type Ia diamond anvil with Raman ultra low fluorescence selection



Second order Raman spectrum of a type Ia diamond anvil with Raman ultra low fluorescence selection

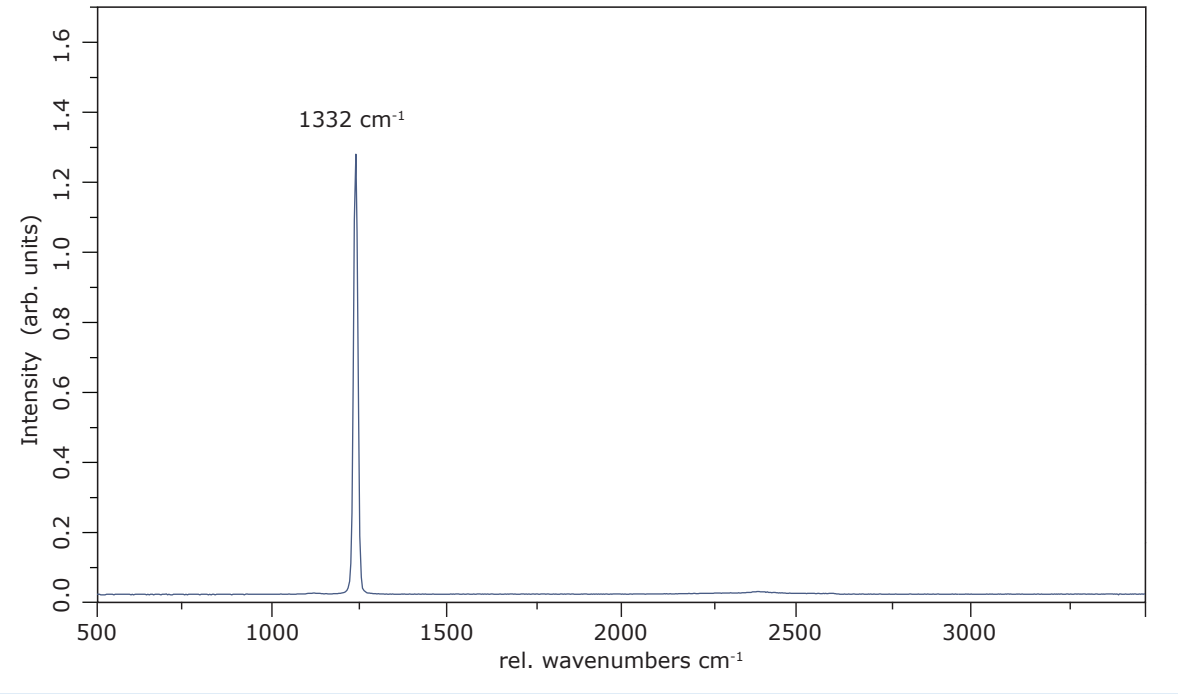